

Fig. 1

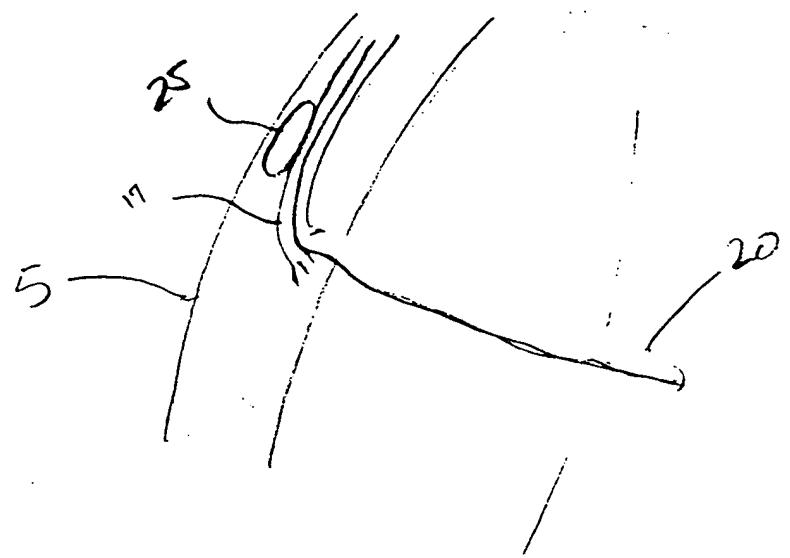


Fig 2.

10060953 - 013006

10060958-013002

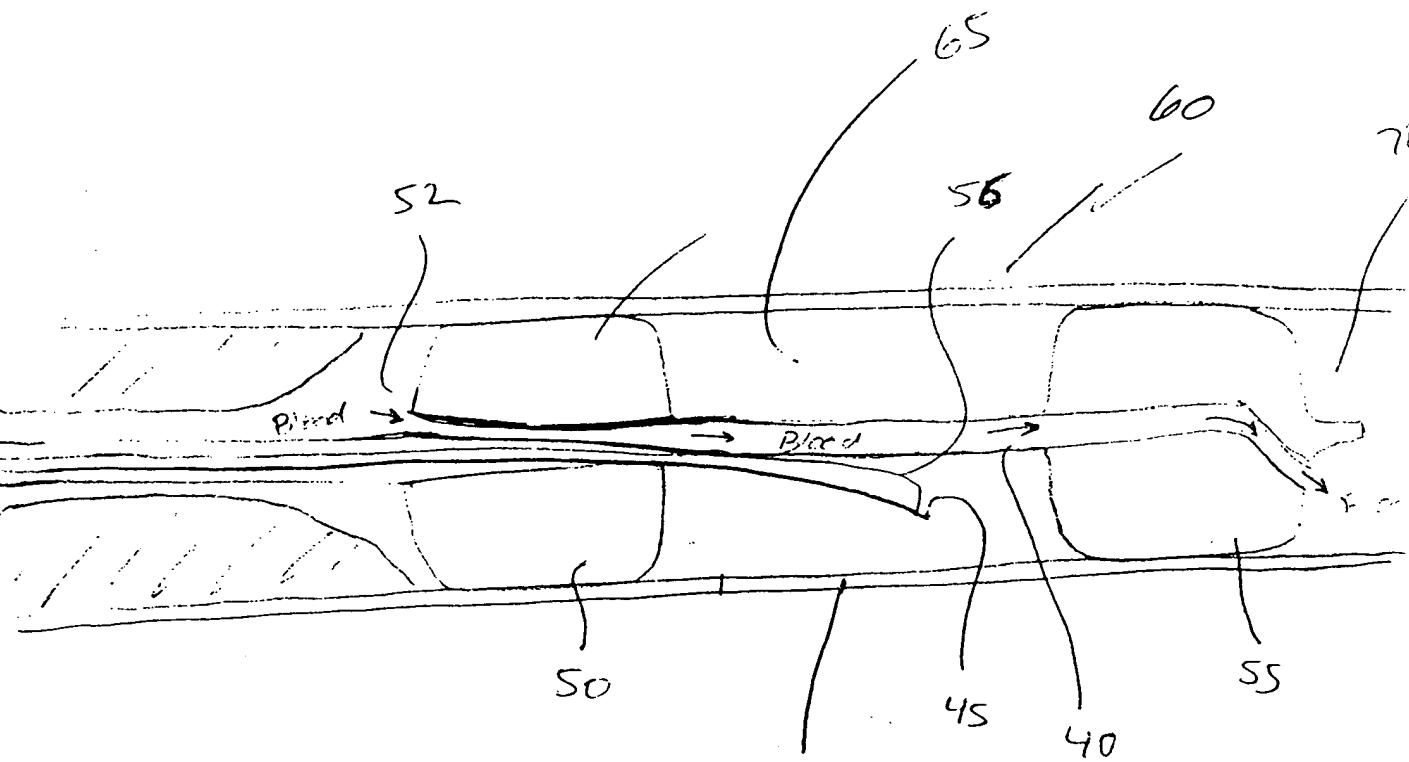


Fig 3

62

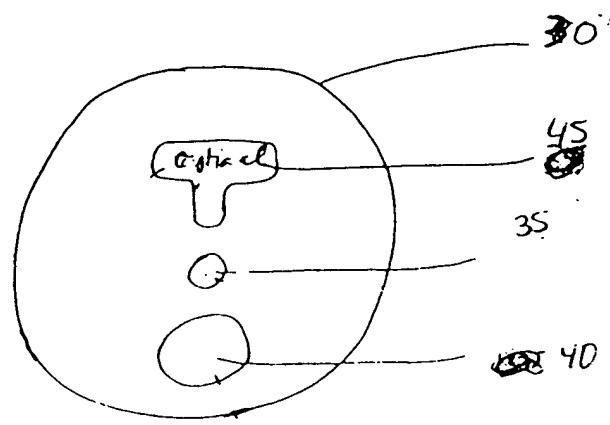


Fig. 34

Heart

20060958 "033002

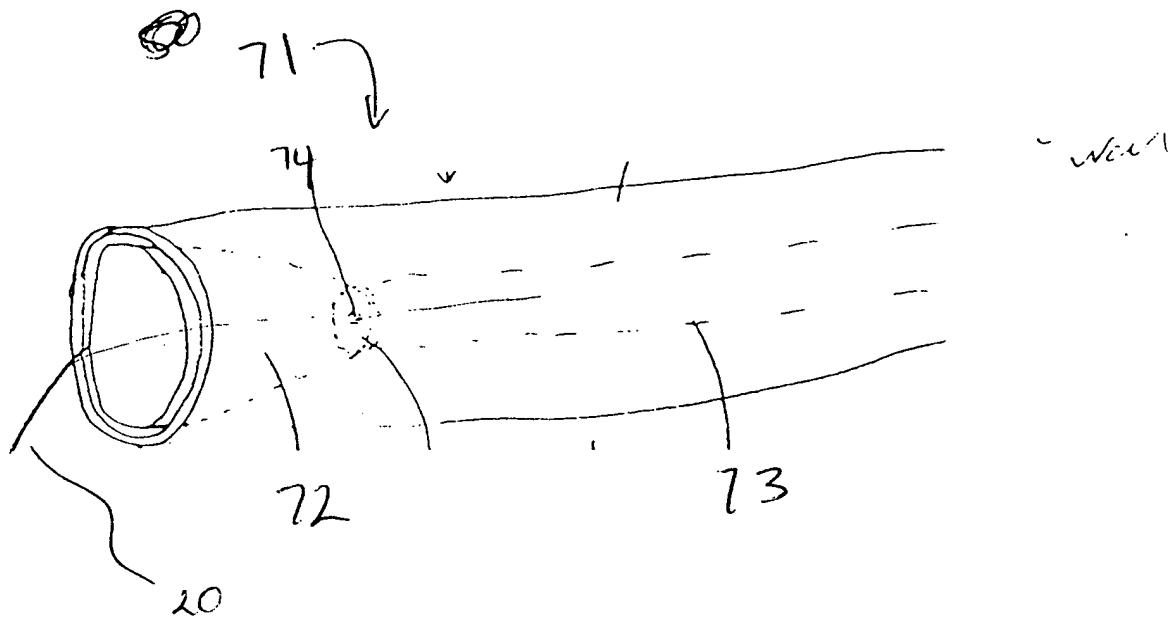


Fig 5

side

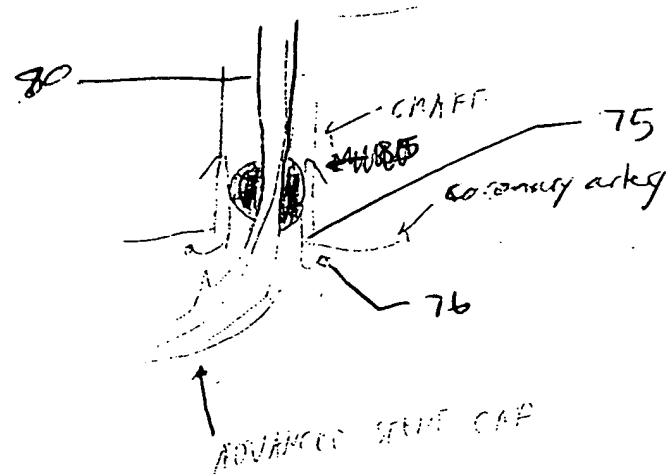


Fig. 5b

10060958 033002

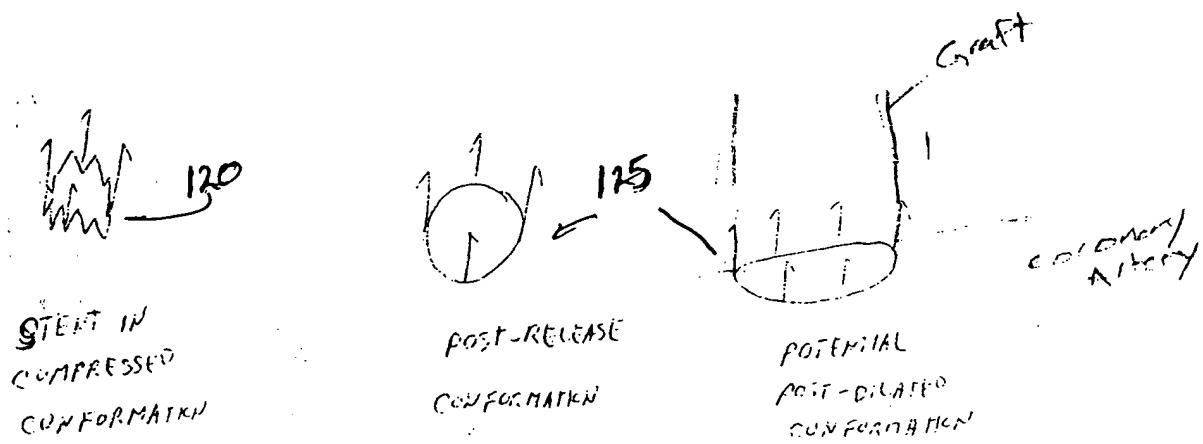


Fig. 5c

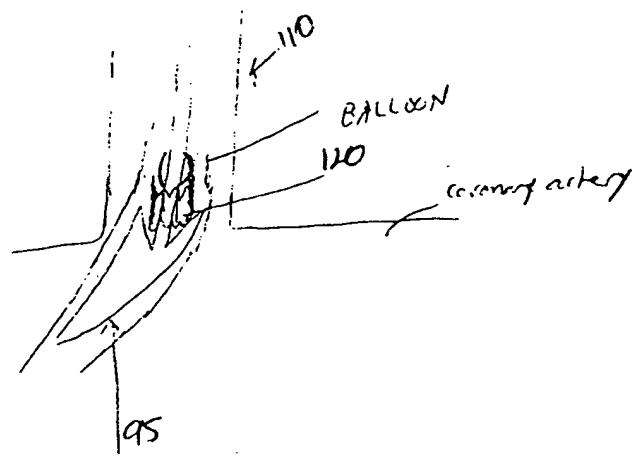


Fig. 8

310060958 - 043002

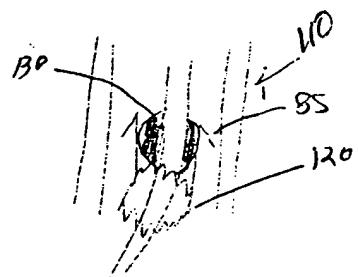


Fig. 89

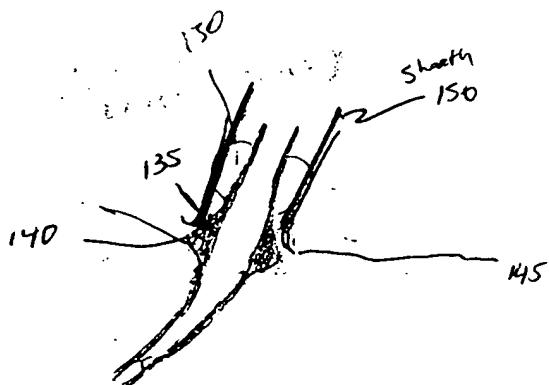


Fig. 810

200 165 110
200 165 110
45 152 85 160 250
coronary artery

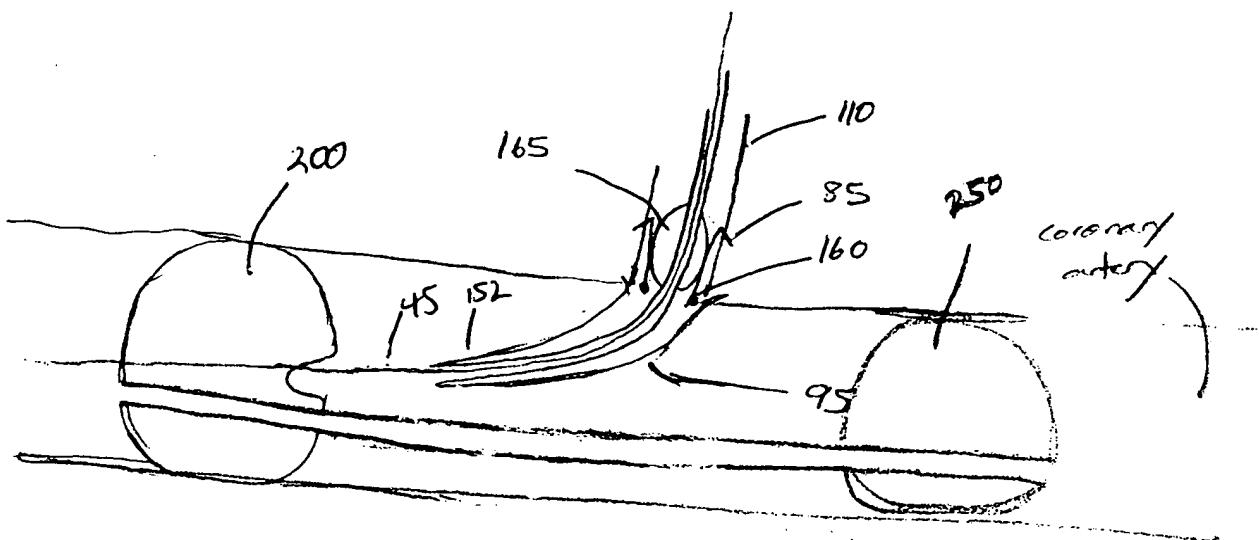


Fig. 11

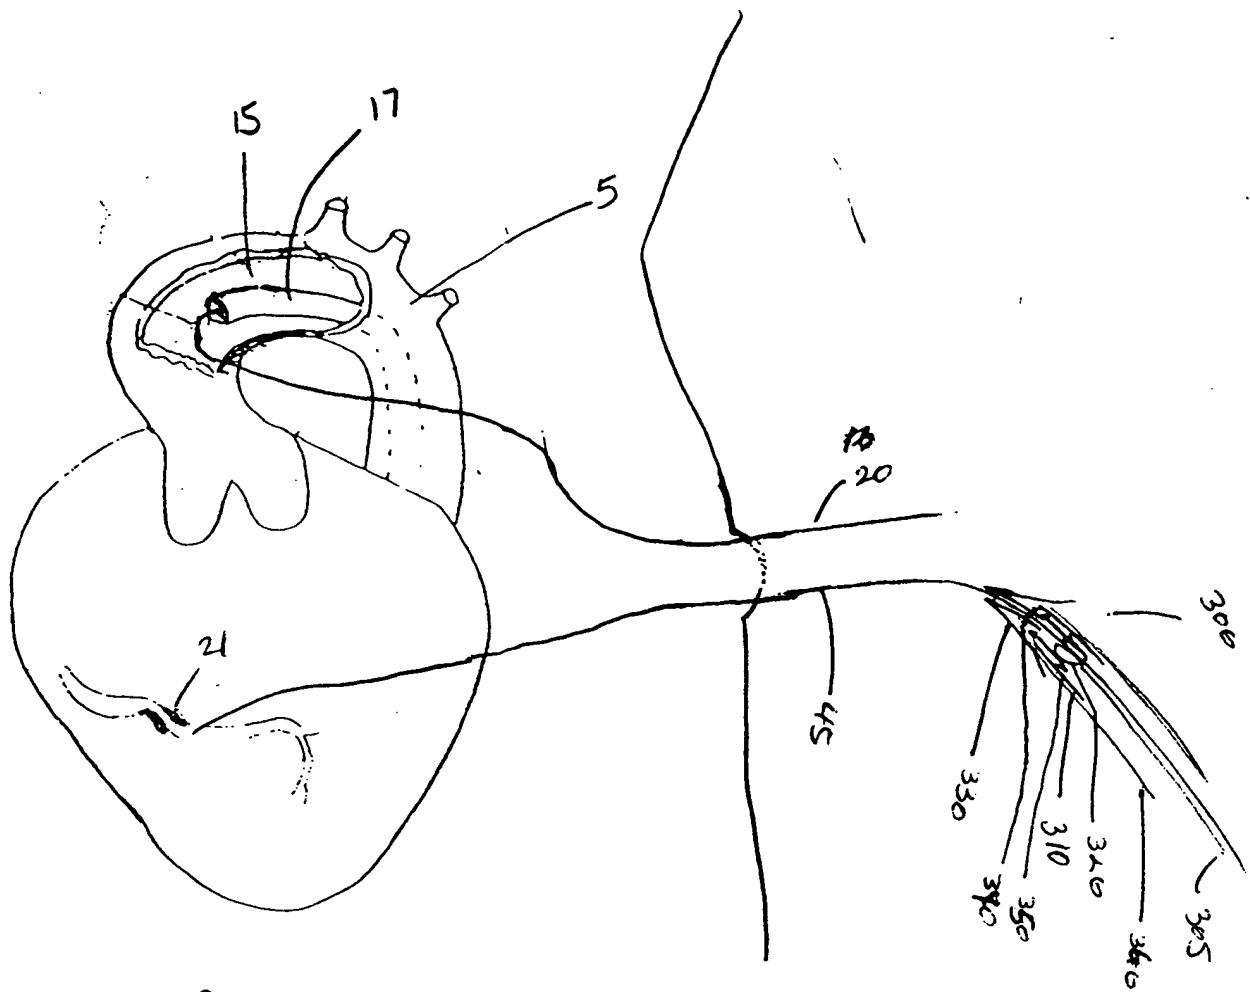


Fig. 12

30050958 01.3002

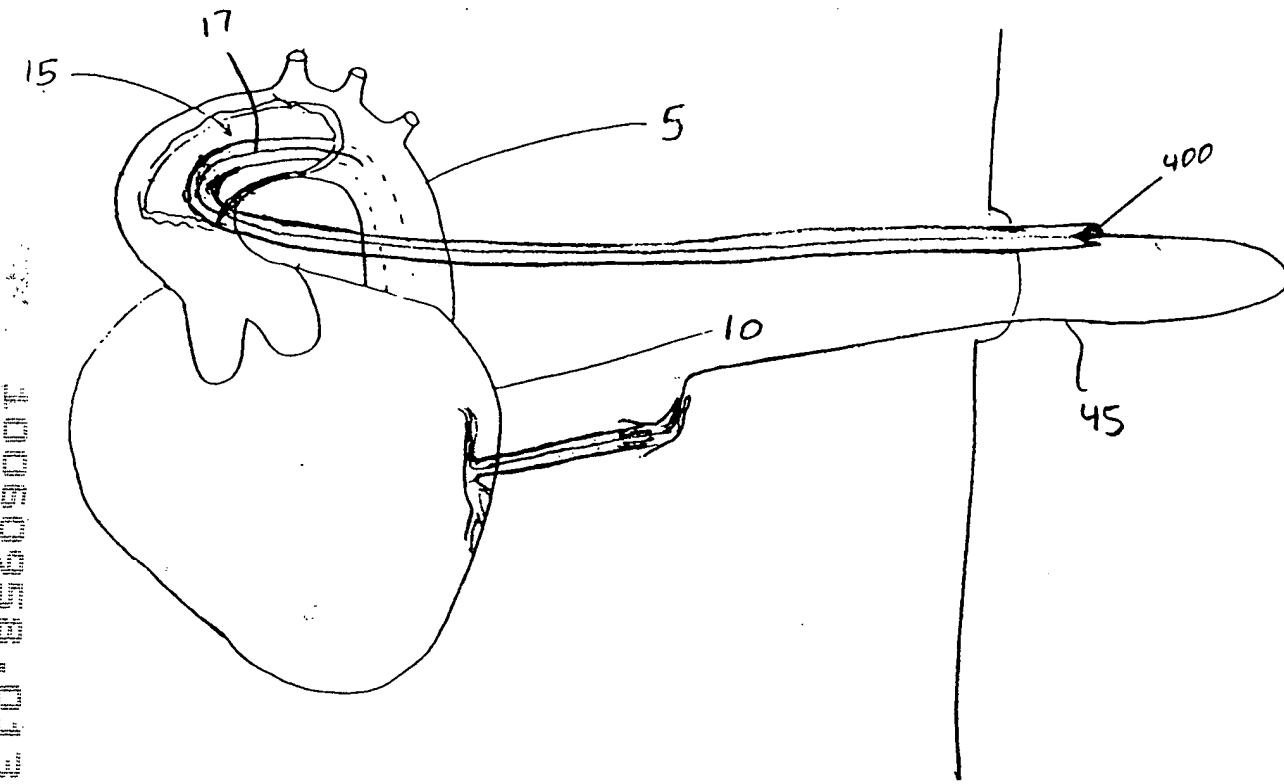


Fig. 1213

1213
Schematic drawing of a probe
for measuring the
concentration of
a radioactive tracer
in a liquid medium
in a flow system

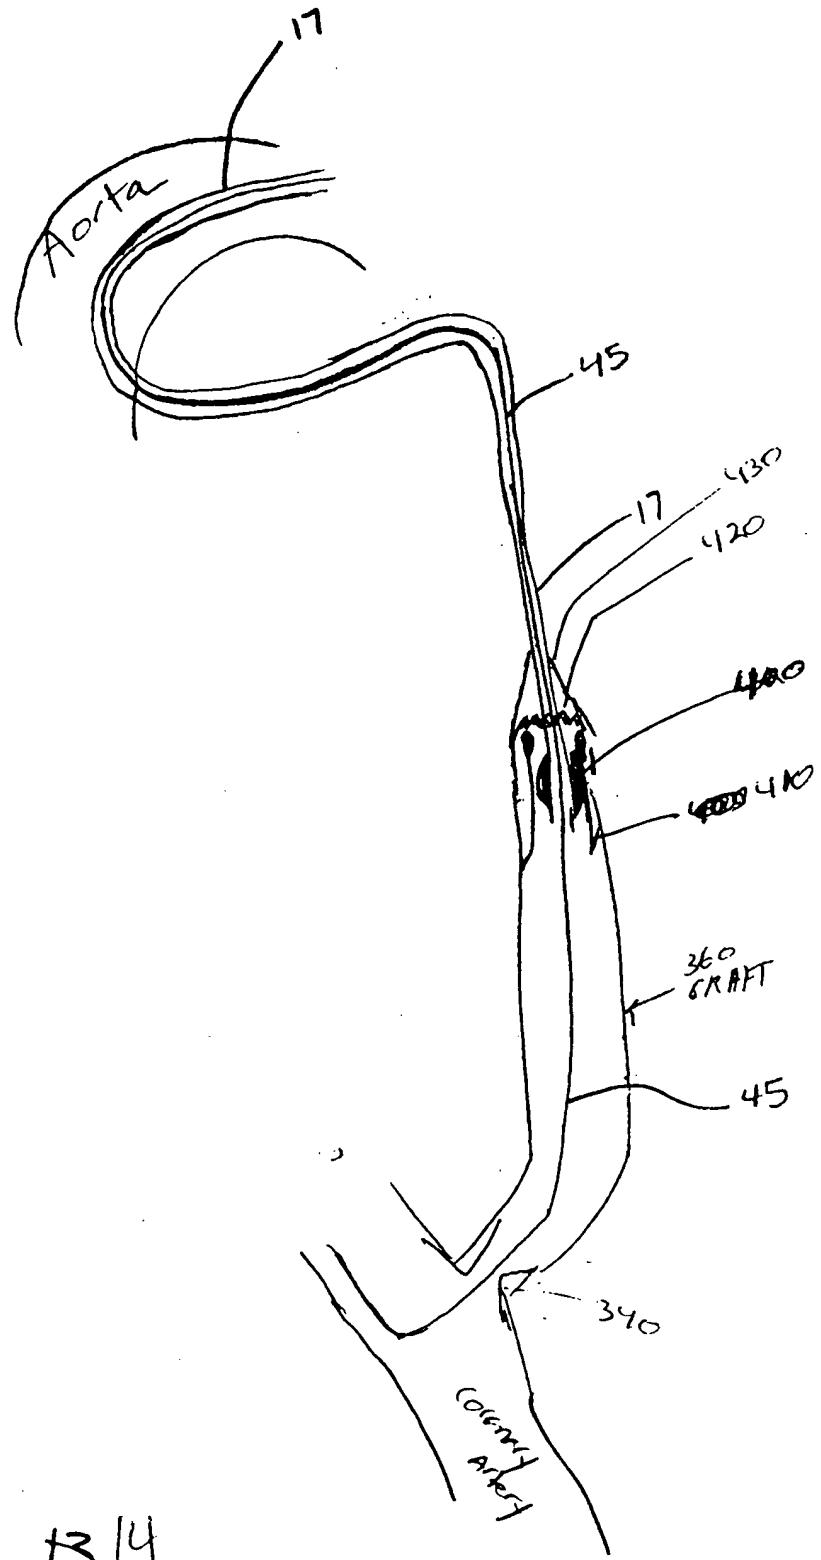


Fig. B.14

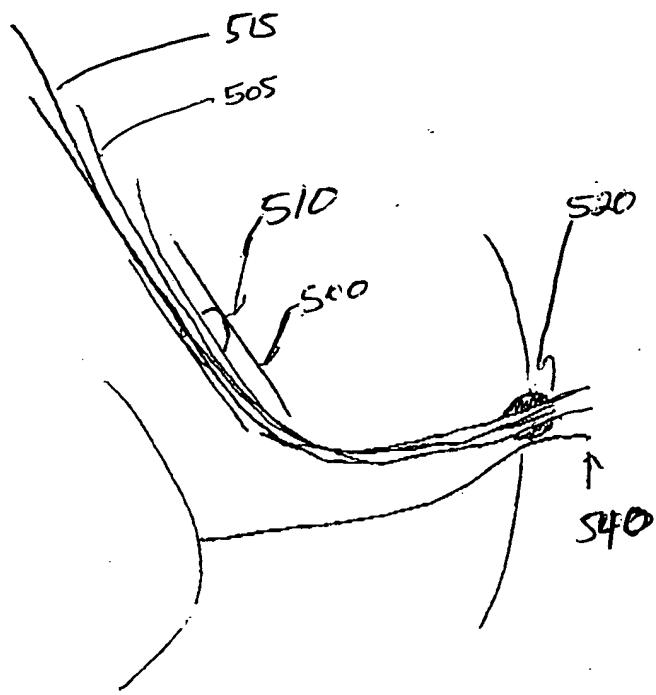


Fig. 15

1.0060958 - 0.13002

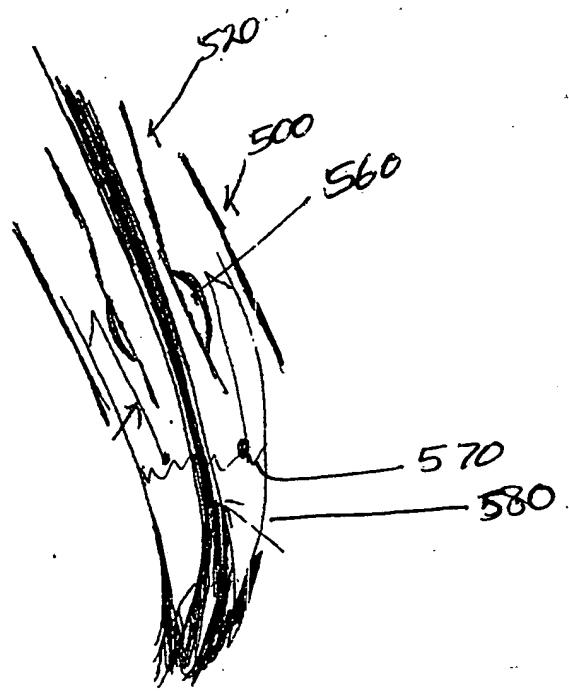


Fig. 16

20050958 013002

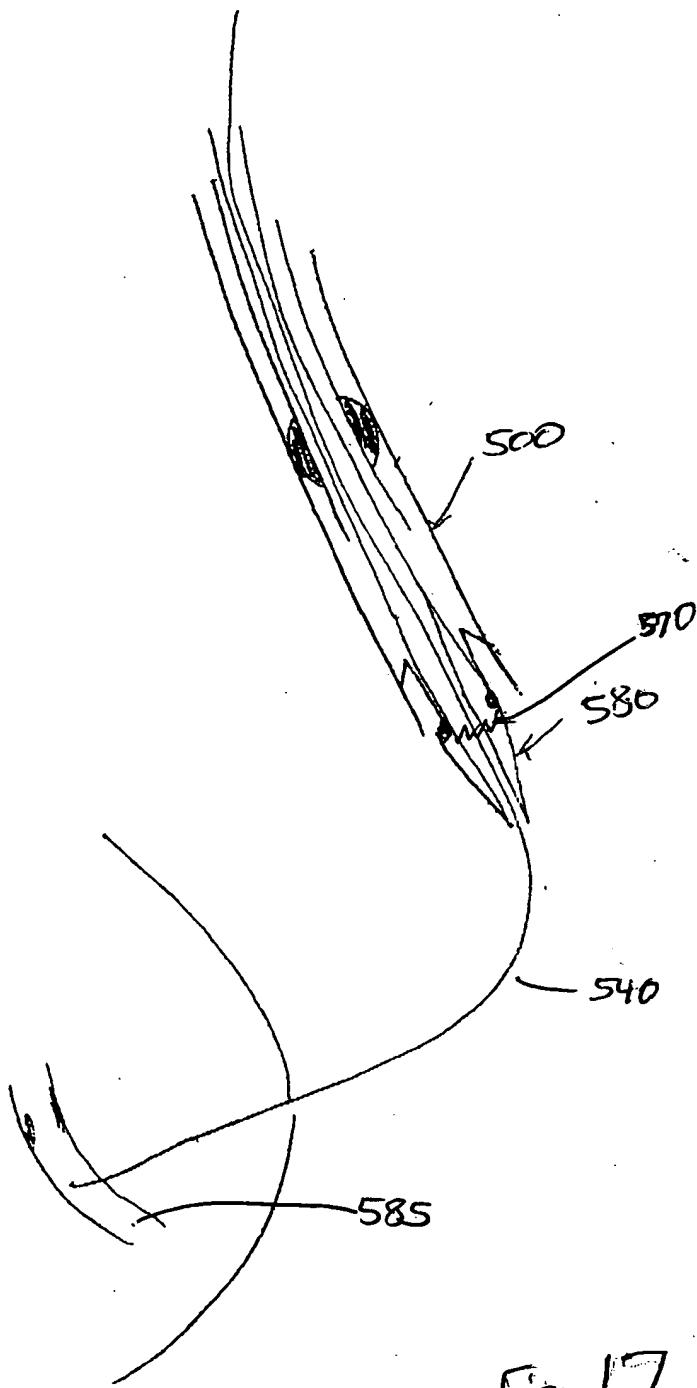


Fig. 17

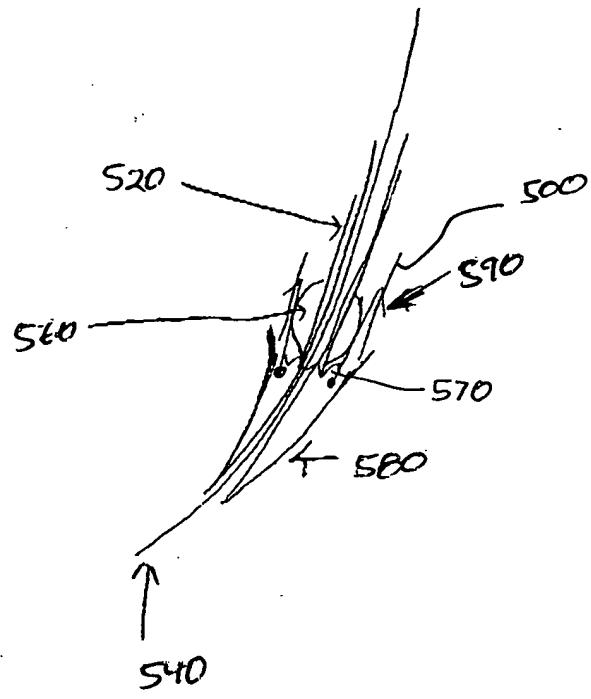


Fig. 18